



PROTECTION & RELIABILITY
OPTIMIZATION INSTRUMENTS

A CTC COMPANY

P R O D U C T M A N U A L

Power Supply



PS12A

12-Channel Rack Mountable Power Supply

CONTENTS

SECTION 1: OVERVIEW.....	4
Introduction	4
Specifications	5
Environmental.....	5
Electrical.....	5
Physical.....	5
SECTION 2: INSTALLATION	6
Description.....	6
SECTION 3: OPERATION	8
Operating Procedure.....	8
SECTION 5: MAINTENANCE.....	14
Maintenance	14
General.....	14
Warranty	14

FIGURES

Figure 1 – PS12A Layout Diagram	7
Figure 2 – PS12A Terminal Block Layout.....	7
Figure 3 – Constant Current Circuit	10

SECTION 1: OVERVIEW

Introduction

PRO PS12A power unit is a 19 inch wide by 1 3/4 high rack mountable, line powered current source power units designed to power 12 channels of regulated current style sensors and in-line charge amplifiers.

NOTE: SENSORS may refer to accelerometers, pressure sensors, hammers and force transducers, etc. The words SENSOR and TRANSDUCER are used interchangeably in this guide.

PRO model PS12A can support up to 12 channels, simultaneously. The sensor signal, riding atop an approximate +12 volt bias level is decoupled from this DC bias by use of a 10 μ F coupling capacitor for each channel.

The PS12A has a sturdy, powder-coated aluminum case that fits standard 19" racks. The front panel has a convenient switchable output BNC to monitor a single channel at a time. The switch also selects the channel of the easy to read 7 segment bias display. All channels have a red-green LED sensor condition indicator light.

On the Back Panel, there are 12 sensor BNC's, as well as 12 output BNC's. In addition there are terminal block inputs that can be used for both the sensors and outputs, in lieu of BNC jacks.

SECTION 1: OVERVIEW

Specifications

RACK MOUNTED POWER SUPPLY

SPECIFICATION	VALUE	UNITS
SENSOR SUPPLY CURRENT (Factory set at 5 mA)	2.0 – 10.0	mA
NUMBER OF SENSOR CHANNELS	12	
SENSOR EXCITATION VOLTAGE (COMPLIANCE VOLTAGE)	+24	VDC
VOLTAGE GAIN	UNITY	
FRONT PANEL LED VOLTMETER F.S.	+24 VDC	
OUTPUT COUPLING CAPACITOR	10	μF
COUPLING TIME CONSTANT w/ 10 MΩ LOAD	100	SEC
w/ 1 MΩ LOAD	10	SEC
LOWER -3db FREQUENCY w/ 10 MΩ LOAD	.0016	Hz
w/ 1 MΩ LOAD	.016	Hz
HIGH FREQUENCY RESPONSE	DETERMINED BY SENSOR, CABLE LENGTH AND SIGNAL LEVEL	
ELECTRICAL NOISE, WIDEBAND	150	μV, RMS
SENSOR CONNECTORS, REAR PANEL	BNC, TERMINAL BLOCK	JACK
OUTPUT CONNECTORS REAR PANEL	BNC, TERMINAL BLOCK	JACK
OUTPUT CONNECTOR FRONT PANEL	BNC	JACK
POWER INPUT	FUSED IEC CONNECTOR	SOCKET
POWER REQUIRED	13.0	VA
LINE VOLTAGE REQUIRED	110-220	VAC
SIZE (H x W x D)	1.7 x 19x 6.5 44 x 483 x 171	INCHES MILLIMETERS
WEIGHT	3.7 1.7	POUNDS KILOGRAMS

Table 1. Specifications

SECTION 2: INSTALLATION

Description

These power units contain a regulated DC power supply and constant current circuits which supply constant current DC power to 12 sensor channels. The constant current sources can be individually adjusted to provide from 2 to 20 mA of drive current per channel.

There is also provision for operation from external +24 VDC batteries or DC power packs for use where AC power is not available.

The front panel has 12 red/green LED's so that sensor condition can be determined at a glance. On the rear panel there are 12 Sensor BNC jacks and 12 Output BNC jacks. In addition, there are terminal block inputs that can be used in lieu of BNC's.

A rotary selector switch (12 position) on the front panel allows the monitoring of the DC bias voltage of each sensor. This is a very handy troubleshooting tool for system checks. Readout is by a front panel mounted 3 digit seven segment display. Also connected to this rotary switch is a front panel mounted BNC 'Monitor' jack which allows the user to look at the signal from the sensor connected to the selected channel. In this way each channel's signal may be inspected.

A three position power switch on the front panel selects AC power or Ext DC power with an 'off' position included. The rear panel has a set of twin banana jacks for connection to the external DC power source. The rear panel also contains the fuse holder and the IEC power entry connector.

SECTION 2: INSTALLATION

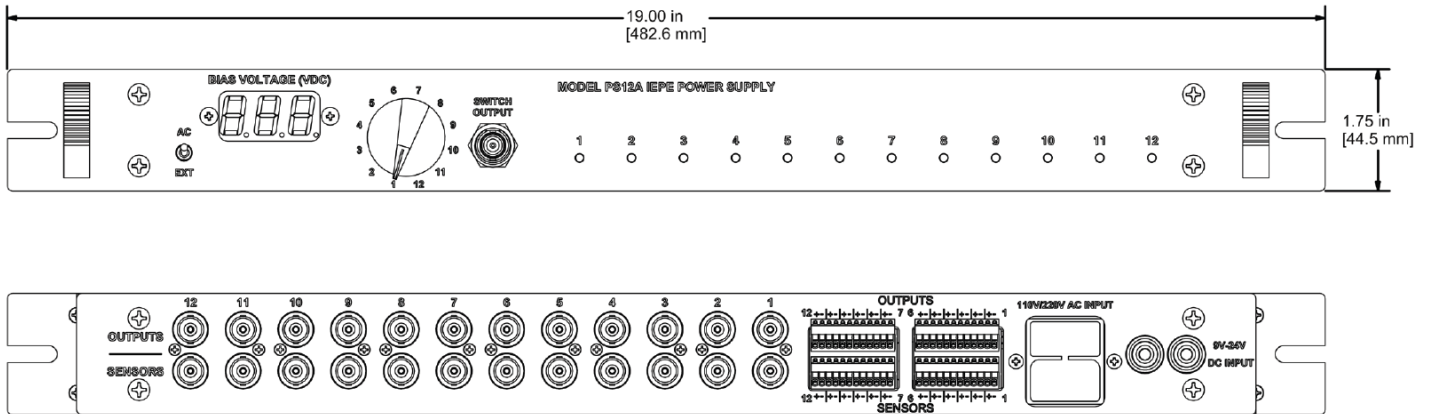


Figure 1. PS12A Power Supply Layout Diagram

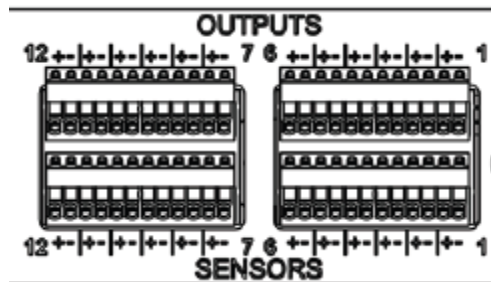


Figure 2. PS12A Terminal Blocks expanded

SECTION 3 : OPERATION

Operating Procedure

OPERATION FROM AC POWER MAINS

Plug the line cord into the appropriate AC power source and move the power switch toggle to the 'AC POWER' position. The indicator lights on the front panel will glow and the voltmeter will indicate full scale with no sensors attached to the sensor jacks.

If these indications are not present, check the fuse at the rear panel. If it is blown, replace it with a 1/4 Amp 3AG fuse only.

OPERATING THE POWER UNIT

Connect the sensor to any one of the 'Sensor' jacks at the rear panel of the power unit. Rotate the channel selector switch on the front panel to the number of the channel into which the sensor has been connected. The front panel 10-segment LED voltmeter should indicate near mid-scale if the sensor and cable are intact and working normally.

In like manner, connect up to the maximum number of sensors and check the bias indications of each for normal operation. If the monitor voltmeter reads full scale, this means:

1. That there is no sensor connected to that channel.
2. The cable to the sensor is open.
3. The sensor is not functioning correctly.

After ensuring that all channels are functioning normally, connect the 'Output' connectors to the readout instrument using the rear sets of output jacks. You are now ready to proceed with the measurement task.

Remember, the rear panel BNC monitor jack allows the user to monitor the signal from any channel selected by the front panel rotary selector switch. Thus, each channel may be monitored for normal operation, even while that channel is being monitored at the rear output jack for that channel.

SECTION 3 : OPERATION

COUPLING TIME CONSTANT

A feature of this system is that power to operate the internal IC in the sensor and the signal from the sensor both flow over the same pair of wires. The DC bias from the sensor amplifier is blocked by a 10 μ F capacitor in the power unit while the AC or dynamic signal is allowed to pass through this blocking capacitor to the output jack.

The value of the coupling capacitor and the resistive load of the readout instrument (in parallel with the pulldown resistor) determine the discharge time constant of the power unit/readout combination and set the low frequency performance of this system.

NOTE: The discharge time constant of the sensor itself must be considered also but for this guide, we will concentrate on the effect of the power unit/readout combination only. The operating guide supplied with the sensor will address the low frequency response of the sensor.

In the PS12 the value of the coupling capacitor is 10 μ F and the pulldown resistor is 1 M Ω . This yields a coupling time constant of:

$$\text{Eq 1. } TC = RC = 1 \times 10^6 \times 10 \times 10^{-6} = 10 \text{ Seconds}$$

SETTING THE CONSTANT CURRENT SENSOR DRIVE CURRENT LEVEL

For most users, this section may be skipped over for now.

The sensor drive current levels are factory set at 5 mA per channel. This is a high enough level for most normal applications and should only be changed when driving very long cables with sensors measuring very high frequencies. For best thermal stability and lowest noise, it is recommended that the sensors operate from 2 to 5 mA of drive current.

These power units use a clamped base transistor circuit as the constant current source. (Figure 3).

The constant current out of the collector is set by the current flowing through the emitter resistor. The base is clamped by the zener/resistor combination to a fixed voltage, and this in turn sets the emitter voltage via the fixed base to emitter voltage characteristic of the transistor. Thus by varying the potentiometer in the emitter circuit, we may set the constant current to any desired level.

SECTION 3: OPERATION

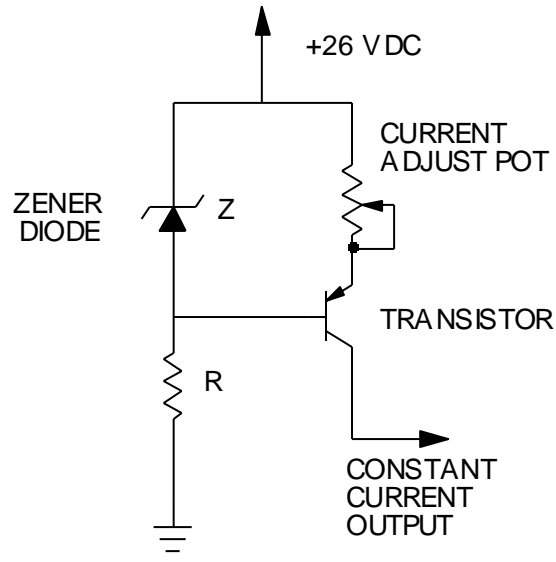


Figure 3. Constant Current Circuit

However, if it is found that the measurement situation calls for higher drive currents, it may be necessary to increase this level. To change the level of sensor drive current, proceed as follows:

1. Remove the top cover by removing the top and bottom screws, as well as the two top mounting screws for the front and back panels.

CAUTION: FOR THE FOLLOWING ADJUSTMENT, USE A NON-METALLIC SCREWDRIVER SINCE VOLTAGES ARE PRESENT IN THIS UNIT WHICH CAN CAUSE ELECTRIC SHOCKS WHICH COULD RESULT IN FATAL INJURY.

2. Set the mA range of a DC milli-ammeter to 20 mA and connect the + lead to the center conductor of a sensor channel and connect the other lead to ground return (the outside shell of the same connector). Read the constant current, then adjust the sensor drive current adjust pot to obtain the desired drive current for that channel. Each channel may be individually adjusted in this manner.

NOTE: Although it may be possible to do so, do not set the drive current above 20 mA. This could be harmful to the sensor.

SENSOR DRIVE VOLTAGE (COMPLIANCE VOLTAGE) SETTING

It should not be necessary under normal conditions to **ever** need to adjust this setting. The output voltage of the DC power supply is regulated by a very stable 3-terminal voltage

SECTION 3 : OPERATION

regulator. This voltage is factory set to provide +24 VDC compliance voltage at +5 mA output level.

EXTERNAL POWER SOURCES

Model PS12A may be powered by an external DC power source such as batteries or a DC power supply. 24 VDC is recommended but voltages down to 18 volts are sufficient. (With voltages as low as +18 volts, the front panel LED voltmeter may not function normally, however the unit will work normally otherwise.)

To use an external supply, connect the leads from the power source to the twin banana plugs at the rear panel. Be sure to observe the proper polarity as marked at the rear panel. A protective diode is built into the PS12A to preclude damage from reverse polarity connection of the power source.

Switch the front panel toggle switch to 'EXT PWR'. With +24 VDC as the power source, it will be noticed that the LED voltmeter may indicate one segment lower than normal when there is no sensor connected to that channel. This is normal and will not affect the operation of the units or the sensors.

When operating from batteries or an external DC power supply, the operation of the sensors and power units, aside from the minor points mentioned, will be the same as with AC power.

The center position of the power toggle switch is the "off" position and should be used when the instrument is not taking data, to prolong battery life.

SECTION 5: MAINTENANCE

Maintenance

Once the product has been installed, minimal maintenance will be required. Basic visual checks to ensure integrity should be made periodically.

General

Under normal usage, no routine maintenance is necessary for these instruments. Should it be necessary to replace the fuse, unplug the unit from the AC line power source, remove the cap from the fuse holder and remove the fuse, Replace only with a 250V/ 0.6A fuse.

Should a problem arise with the power unit, contact the factory for help in analyzing the problem and/or for instructions on sending the unit back for evaluation.

Should the PS12 develop a problem, contact the factory Service Department for help in trouble shooting or for instructions in returning the unit to the factory for evaluation. At this time, a Returned Material Authorization (RMA) number will be assigned to help track the unit through the repair process, should it be necessary to return the unit to the factory.

Warranty

If any PRO product should ever fail, we will repair or replace it at no charge, as long as the product was not subjected to misuse, natural disasters, improper installation or modification which caused the defect.